

C0650 Power Meter



The Appointech C0650 handheld power meters have calibrated outputs at LD wavelengths of 650nm, or other visible wavelengths. The operation is very user-friendly. After turn-on with the ON/OFF switch, the given individual input wavelength is set by pressing the λ -key until the correct value is shown on the LCD display, together with the corresponding input power value. The power unit is normally set in dBm. When the dB/dBm key is pressed for about 3 seconds until dB is flashing on the LCD, the current input power level is taken as the new reference at 0 dB, and the following measurement will be the difference in dB, with respect to the new reference. When in Auto-Off mode, as indicated by a power symbol with a cross on the LCD, the unit will be shut off after about 30 minutes on-time for battery life, in case not in use for a prolonged time. To turn it back on, press the ON/OFF key again. The auto-off feature can be disabled by pressing the Auto-Off key, as indicated by a power symbol without a cross on the LCD. When the battery power is too low to assume proper operation, an empty battery symbol is shown on the LCD display. The included rechargeable battery works with a power adaptor of a USB connector, which is also included. When charging is in OFF-mode, the indicator LED will be on until charging has been completed. An on-site calibration switch is located inside the battery compartment. When the switch is moved to CAL, the unit can be calibrated on-site with respect to the customer's own standard power meter. The power of a stabilized light source of the wavelength to be calibrated is first measured with the standard power meter, then with the power meter to be calibrated. The power reading is changed by pressing the up \blacktriangle and down \blacktriangledown keys until the expected power value is shown on the LCD. The switch has to be moved back to "Normal" after calibration is finished.

Features

- Calibration on-site with customer's own standard if needed
- Display measurement in dB/dBm
- Selection of relative/absolute power measurement
- Resolution 0.01dB; absolute accuracy ± 0.25 dB
- Small size, easy for field applications
- Light weight, about 0.2Kg
- Auto power shut-off can be disabled
- Rechargeable battery, Battery-full and Battery-low indicator

Applications


- Power measurements
- Transmission loss measurement
- Calibration of optical receivers

C0650 Power Meter

Specifications


Detector Material	Si
Calibration Wavelengths	650nm, or customer specified visible wavelengths
Power Range	+3 to -60 dBm or +23 to -40 dBm
Polarization Dependence	< 0.1 dB
Absolute Accuracy	±0.25dB under calibrated conditions
Linearity	±0.05dB
Display	LCD displays power in selected unit, wavelength. Warning symbol for low battery, Auto-Off Enable/disable
Calibration Data	Data stored in non-volatile memory
Functions	ON/OFF: power switch; Auto-Off: enable/disable switch λ-key: input wavelength selection dB/dBm-key: power unit selection, and new power reference set On-site calibration up-down keys Battery level indicator
Optical Connector Interface	FC or ST or SC or universal, adapter for other connector available
Environmental: Operation Temp, Humidity Storage Temp, Humidity	-15°C to +50°C, 0-95% RH (non-condensing) -35°C to +70°C, 0-95% RH (non-condensing)
Power	Rechargeable Lithium battery, works continuously for more than 20 hrs after 2-hrs full charge
Dimensions (Length x Width x Height)	16x7x3 cm (measured without case)
Weight (w/ batteries)	<0.2Kg

Ordering information

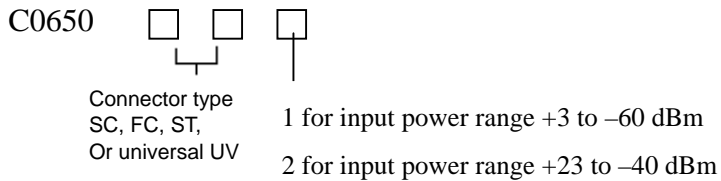

Options: Standard Multi-units Carrying Case
Heavy-Duty Multi-units Carrying Case
Receptacle Converters

C0650 Power Meter

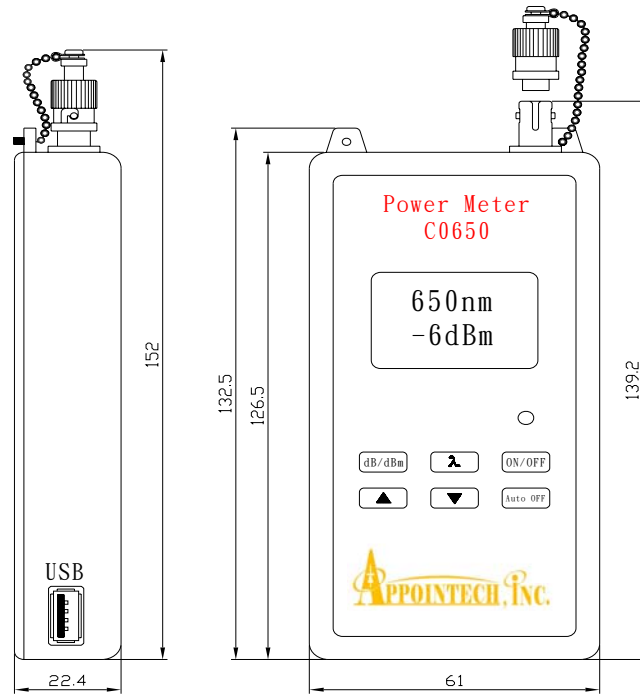

C0650 Power Meter

Unit:mm

